

Non-destructive testing — Ultrasonic examination —

Part 2: Sensitivity and range setting

The European Standard EN 583-2:2001 has the status of a
British Standard

ICS 19.100

NO COPYING WITHOUT BSI PERMISSION EXCEPT AS PERMITTED BY COPYRIGHT LAW



National foreword

This British Standard is the official English language version of EN 583-2:2001.

The UK participation in its preparation was entrusted to Technical Committee WEE/46, Non-destructive testing, which has the responsibility to:

- aid enquirers to understand the text;
- present to the responsible European committee any enquiries on the interpretation, or proposals for change, and keep the UK interests informed;
- monitor related international and European developments and promulgate them in the UK.

A list of organizations represented on this committee can be obtained on request to its secretary.

Cross-references

The British Standards which implement international or European publications referred to in this document may be found in the BSI Standards Catalogue under the section entitled "International Standards Correspondence Index", or by using the "Find" facility of the BSI Standards Electronic Catalogue.

A British Standard does not purport to include all the necessary provisions of a contract. Users of British Standards are responsible for their correct application.

Compliance with a British Standard does not of itself confer immunity from legal obligations.

This British Standard, having been prepared under the direction of the Engineering Sector Committee, was published under the authority of the Standards Committee and comes into effect on 15 March 2001

Summary of pages

This document comprises a front cover, an inside front cover, the EN title page, pages 2 to 44, an inside back cover and a back cover.

The BSI copyright date displayed in this document indicates when the document was last issued.

Amendments issued since publication

Amd. No.	Date	Comments

© BSI 03-2001

ISBN 0 580 37026 7

EUROPEAN STANDARD

EN 583-2

NORME EUROPÉENNE

EUROPÄISCHE NORM

January 2001

ICS 19.100

English version

Non-destructive testing — Ultrasonic examination — Part 2: Sensitivity and range setting

Essais non destructifs — Contrôle ultrasonore —
Partie 2: Réglage de la sensibilité et de la base de temps

Zerstörungsfreie Prüfung — Ultraschallprüfung —
Teil 2: Empfindlichkeits- und Entfernungseinstellung

This European Standard was approved by CEN on 5 January 2001.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the Management Centre or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the Management Centre has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Czech Republic, Denmark, Finland, France, Germany, Greece, Iceland, Ireland, Italy, Luxembourg, Netherlands, Norway, Portugal, Spain, Sweden, Switzerland and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION
COMITÉ EUROPÉEN DE NORMALISATION
EUROPÄISCHES KOMITEE FÜR NORMUNG

Management Centre: rue de Stassart, 36 B-1050 Brussels

© 2001 CEN All rights of exploitation in any form and by any means reserved
worldwide for CEN national Members.

Ref. No. EN 583-2:2001 E

Contents

	Page
Foreword	3
1 Scope	4
2 Normative references	4
3 General	4
3.1 Quantities and symbols.....	4
3.2 Test objects, reference blocks and reference reflectors.....	4
3.3 Categories of test objects.....	4
3.4 Contouring of probes.....	5
4 Determination of probe index and beam angle	7
4.1 General	7
4.2 Flat probes	7
4.3 Probes curved longitudinally	7
4.4 Probes curved transversely.....	10
4.5 Probes curved in two directions	13
4.6 Probes for use on materials other than non-alloy steel	13
5 Range setting	13
5.1 General	13
5.2 Reference blocks and reference reflectors.....	14
5.3 Straight beam probes.....	14
5.4 Angle beam probes.....	14
5.5 Alternative range settings for angle beam probes.....	15
6 Sensitivity setting and echo height evaluation	17
6.1 General	17
6.2 Angle of impingement	18
6.3 Distance Amplitude Curve (DAC) technique	18
6.4 Distance Gain Size (DGS) technique	21
6.5 Transfer correction	26
Annex A (normative) Table A.1 — Quantities and symbols	30
Annex B (normative) Reference blocks and reference reflectors	32
Annex C (normative) Determination of sound path distance and impingement angle in concentrically curved objects	35
Annex D (informative) General DGS diagram	39
Annex E (informative) Determination of contact transfer correction factors	41
Bibliography	44

Foreword

This European Standard has been prepared by Technical Committee CEN/TC 138, Non-destructive testing, the Secretariat of which is held by AFNOR.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by July 2001, and conflicting national standards shall be withdrawn at the latest by July 2001.

This European Standard has been prepared under a mandate given to CEN by the European Commission and the European Free Trade Association. This European Standard is considered to be a supporting standard to those application and product standards which in themselves support an essential safety requirement of a New Approach Directive and which make reference to this European Standard.

This standard consists of the following parts:

- EN 583-1, *Non-destructive testing — Ultrasonic examination — Part 1: General principles.*
- EN 583-2, *Non-destructive testing — Ultrasonic examination — Part 2: Sensitivity and range setting.*
- EN 583-3, *Non-destructive testing — Ultrasonic examination — Part 3: Transmission technique.*
- EN 583-4, *Non-destructive testing — Ultrasonic examination — Part 4: Examination for discontinuities perpendicular to the surface.*
- EN 583-5, *Non-destructive testing — Ultrasonic examination — Part 5: Characterization and sizing of discontinuities.*
- ENV 583-6, *Non-destructive testing — Ultrasonic examination — Part 6: Time-of-flight diffraction technique as a method for detection and sizing of discontinuities.*

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Czech Republic, Denmark, Finland, France, Germany, Greece, Iceland, Ireland, Italy, Luxembourg, Netherlands, Norway, Portugal, Spain, Sweden, Switzerland and the United Kingdom.

1 Scope

This part of the standard specifies the general rules for setting the time base range and sensitivity (i. e. gain adjustment) of a manually operated ultrasonic flaw detector with A-scan display in order that reproducible measurements may be made of the location and echo height of a reflector.

It is applicable to techniques employing a single contact probe with either a single or twin transducers, but excludes immersion technique and techniques employing more than one probe.

2 Normative references

This European Standard incorporates, by dated or undated reference, provisions from other publications. These normative references are cited at the appropriate places in the text and the publications are listed hereafter. For dated references, subsequent amendments to or revisions of any of these publications apply to this European Standard only when incorporated in it by amendment or revision. For undated references the latest edition of the publication referred to applies (including amendments).

- EN 12223, *Non-destructive testing — Ultrasonic examination — Specification for calibration block No. 1.*
- EN 27963, *Welds in steel — Calibration block No. 2 for ultrasonic examination of welds (ISO 7963:1985).*
- EN 12668-3, *Non-destructive testing — Characterization and verification of ultrasonic examination equipment — Part 3: Combined equipment.*

3 General

3.1 Quantities and symbols

A full list of the quantities and symbols used throughout this part of the standard is given in annex A.











3.2 Test objects, reference blocks and reference reflectors

Requirements for geometrical features of test objects, reference blocks and reference reflectors in general are contained in annex B.

3.3 Categories of test objects

The requirements for range and sensitivity setting will depend on the geometrical form of the test object. Five categories of test objects are defined in Table 1.

Table 1 — Categories of test objects

Class	Feature	Section in X-direction	section in Y-direction
1	Plane parallel surfaces (e.g. plate/sheet)		
2	Parallel, uniaxially curved surfaces (e.g. tubes)		
3	Parallel surfaces curved in more than one direction (e.g. dished ends)		
4	Solid material of circular cross section (e.g. rods and bars)		
5	Complex shapes (e.g. nozzles, sockets)		

3.4 Contouring of probes

Contouring of the probe shoe, for geometry categories 2 to 5, may be necessary to avoid probe rocking, i.e. to ensure good, uniform, acoustic contact and a constant beam angle in the test object. Contouring is only possible with probes having a hard plastic stand-off (normally twin-transducer straight beam probes or angle beam probes with wedges).

The following conditions for the different geometric categories exist (see Table 1 and Figure 1):

- category 1: No probe contouring necessary for scanning in either X- or Y-direction;
- categories 2 and 4: scanning in X-direction: Probe face longitudinally curved,
scanning in Y-direction: Probe face transversely curved;
- categories 3 and 5: scanning in either X or Y-direction:
Probe face longitudinally and transversely curved.

The use of contoured probes necessitates setting the range and sensitivity on reference blocks contoured similarly to the test object, or the application of mathematical correction factors.

When using equations (1) or (2), problems due to low energy transmission or beam misalignment are avoided.

3.4.1 Longitudinally curved probes

3.4.1.1 Convex scanning surface

For scanning on convex surfaces the probe face shall be contoured when the diameter of the test object, D_{obj} , is below ten times the length of the probe shoe, l_{ps} (see Figure 1):

$$D_{obj} < 10l_{ps} \quad (1)$$

3.4.1.2 Concave scanning surface


On a concave scanning surface the probe face shall always be contoured, unless adequate coupling can be achieved due to very large radii of curvature.

3.4.2 Transversely curved probes

3.4.2.1 Convex scanning surface

For scanning on convex surfaces the probe face shall be contoured when the diameter of the test object, D_{obj} , is below ten times the width of the probe shoe, w_{ps} (see Figure 1):

$$D_{obj} < 10w_{ps} \quad (2)$$

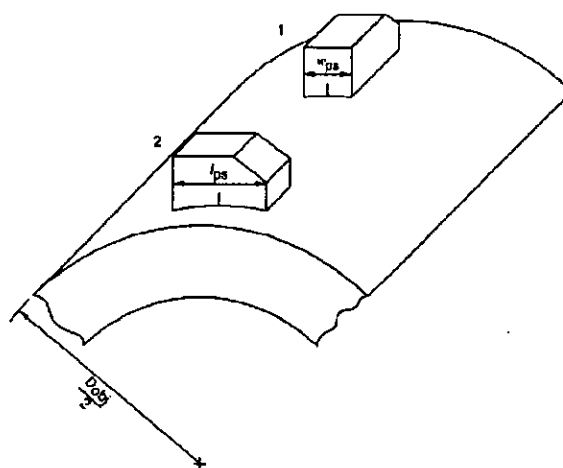

Key

- 1 Transversely curved
- 2 Longitudinally curved

Figure 1 — Length, l_{ps} , and width, w_{ps} , of probe shoe in direction of curvature of the test object

3.4.2.2 Concave scanning surface

On a concave scanning surface the probe face shall always be contoured, unless adequate coupling can be achieved due to very large radii of curvature.

3.4.3 Longitudinally and transversely curved probes

The probe face shall fulfil the requirements of 3.4.1 and 3.4.2.

4 Determination of probe index and beam angle

4.1 General

For straight beam probes there is no requirement to measure probe index and beam angle as it is assumed that the probe index is in the centre of the probe face and the angle of refraction is zero degrees.

When using angle probes, these parameters shall be measured in order that the position of a reflector in the test object can be determined in relation to the probe position. The techniques and reference blocks employed depend on the contouring of the probe face.

Measured beam angles depend on the sound velocity of the reference block used. If the block is not made of non-alloy steel its velocity shall be determined and recorded.

4.2 Flat probes

4.2.1 Calibration block technique

Probe index and beam angle shall be determined using Calibration Block No. 1 or Calibration Block No. 2 according to the specifications given in EN 12223 or EN 27963 respectively, depending on the size of the probe.

4.2.2 Reference block technique

An alternative technique using a reference block containing at least 3 side-drilled holes as given in EN 12668-3 may be used.

4.3 Probes curved longitudinally

4.3.1 Mechanical determination

Before contouring the probe face, the probe index and beam angle shall be measured as described in 4.2.1.

The incident angle at the probe face (α_d) shall be calculated from the measured beam angle (α) and a line, originating from the probe index and parallel to the incident beam, shall be marked on the side of the probe, as shown in Figure 2.

The incident angle is given by equation 3:

$$\alpha_d = \arcsin \left(\frac{c_d}{c_t} \sin \alpha \right) \quad (3)$$

where:

- c_d is the longitudinal wave velocity in the probe wedge (normally 2 730 m/s for acrylic glass);
- c_t is the transverse wave velocity in the test object (3 255 m/s \pm 15 m/s for non-alloy steel).

After contouring, the probe index will have moved along the marked line, and its new position can be measured by mechanical means directly on the probe housing, as shown in Figure 2.


The beam angle shall be determined by maximizing the echo from a side-drilled hole satisfying the conditions given in annex B. The beam angle may then be measured directly on the test object, on the reference block, or on a scale drawing. See Figure 3.

Alternatively, the beam angle may be determined by calculation on the basis of the sound path length measured on the reference block by mechanical means, using equation (4). This may be accomplished together with the range setting as described in 5.4.4.

$$\alpha = \arccos \left\{ \frac{\left[(D_{SDH}/2)^2 + s^2 - t^2 + sD_{SDH} + tD_{Obj} \right]}{D_{Obj} [s + (D_{SDH}/2)]} \right\} \quad (4)$$

The symbols used in this equation are illustrated in Figure 3.

The radius of curvature of the surface used for the calibration shall be within ± 10 % of that of the test object.

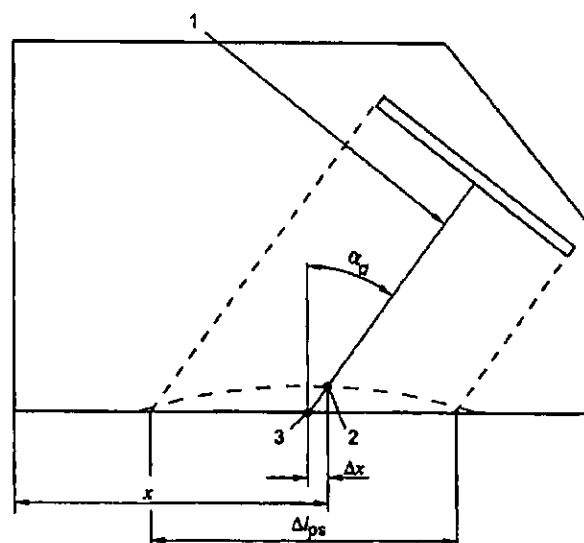

Key

- 1 Marked line for index shift
- 2 Index point after contouring
- 3 Index point before contouring

Figure 2 — Determination of Index shift for longitudinally curved probes

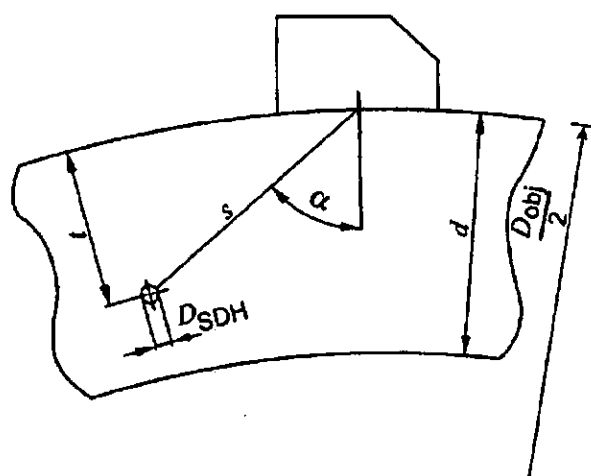


Figure 3 — Determination of beam angle α for a longitudinally contoured probe face

4.3.2 Reference block technique

This is similar to that referenced in 4.2.2, except that the test block shall have a radius of curvature within $\pm 10\%$ of that of the test object.

4.4 Probes curved transversely

4.4.1 Mechanical determination

Before contouring the probe face the probe index and beam angle shall be measured as described in 4.2.

After contouring, either:

i) a line representing the incident beam, originating from the probe index, shall be marked on the side of the probe. The new position of the probe index shall be measured on the side of the probe as shown in Figure 4;

ii) the shift in probe index position (Δx) shall be calculated using equation 5:

$$\Delta x = g \tan (\alpha_d) \quad (5)$$

The symbols in this equation are illustrated in Figure 4;

iii) for acrylic glass wedges ($c_d = 2\,730$ m/s) and non-alloy steel test objects ($c_t = 3\,255$ m/s) the shift in the probe index position (Δx), for the three most commonly used beam angles, shall be read from Figure 5 in relation to the depth of contouring (g).

The beam angle should not change during contouring.


However, if it is not known, or there is any variation in the depth of contouring along the length of the probe, it shall be measured on a suitably contoured reference block using a side drilled hole satisfying the conditions given in annex B. The beam angle shall be determined by:

i) drawing a straight line between the hole and the probe index on a scale drawing;

or

ii) calculation using, for example, equation (6) for the set-up illustrated in Figure 6:

$$\alpha = \left(\frac{\arctan A' + x - q}{t} \right) \quad (6)$$

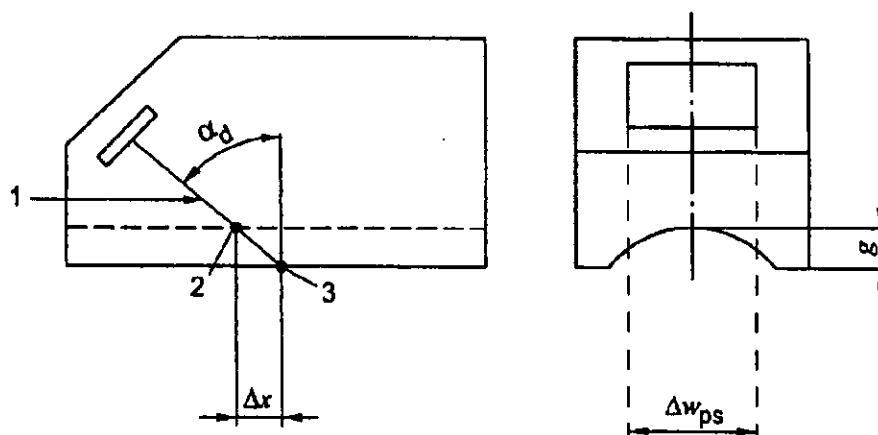

Key

- 1 Marked line for index shift
- 2 Index point after contouring
- 3 Index point before contouring

Figure 4 — Determination of index shift for transversely curved probes

4.4.2 Reference block technique

This technique is similar to that referenced in 4.2.2 except that the test block shall be curved transversely in relation to the probe, and shall have a radius of curvature not exceeding 10 % higher, or 30 % lower, than that of the test object.

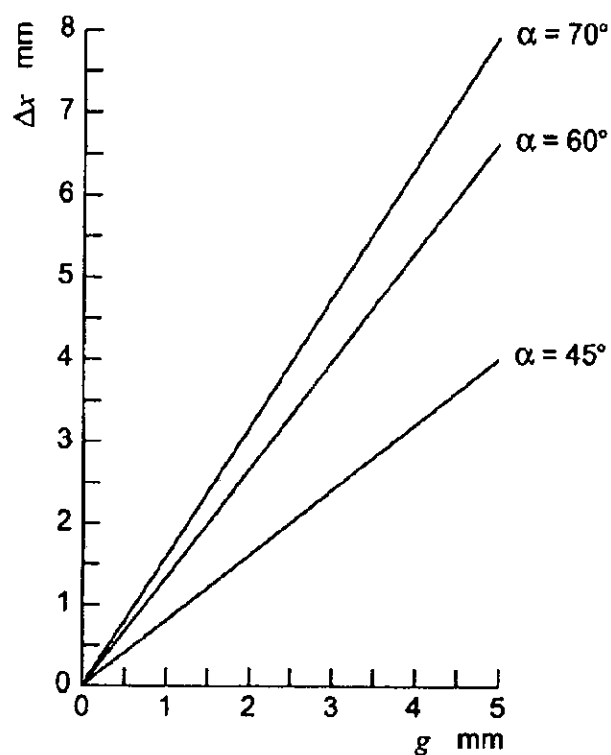


Figure 5 — Probe index shift, Δx , for delay paths in acrylic glass

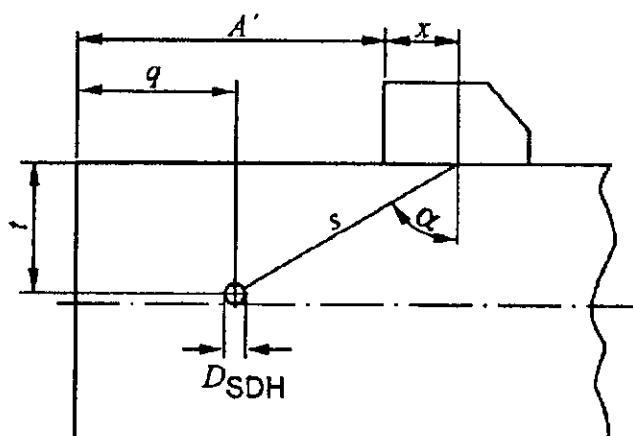


Figure 6 — Determination of beam angle using a side-drilled hole

4.5 Probes curved in two directions

Unless the need for multiaxial curving of the probe face can be avoided, e.g. by use of smaller probes, the procedures specified in 4.2, 4.3 and 4.4 shall be followed as appropriate.

4.6 Probes for use on materials other than non-alloy steel

If the sound velocity in the material under test is markedly different from that in non-alloy steel, the position of the probe index and the beam angle will be significantly changed. The use of the radii on Calibration Block No. 1 or Calibration Block No. 2 may lead to confusing results.

If the sound velocity is known, the beam angle can be calculated as follows:

$$\alpha_t = \arcsin \left(\frac{c_t}{c_r} \sin \alpha_r \right) \quad (7)$$

where:

- α_r is the beam angle in a non-alloy steel reference block;
- α_t is the beam angle in the test object;
- c_t is the transverse wave velocity in the test object;
- c_r is the transverse wave velocity in the non-alloy steel reference block
(3 255 m/s \pm 15 m/s).

If the sound velocity is not known, the beam angle can be determined using an echo from a side-drilled hole in a sample of the material, as illustrated in Figure 6, or as described in 4.3.1 or in 4.4.1, as appropriate.

5 Range setting

5.1 General

For all tests using the pulse echo technique, the time base of the ultrasonic instrument shall be set to indicate, on the screen, the sound propagation time, or, more usually, some parameters directly related to it. Such parameters may be the sound path length of a reflector, its depth below the test surface, its projection distance, or its shortened projection distance, see Figure 7. Unless otherwise noted, the procedures described below refer to setting the time base in terms of the sound path length (an echo travels this path twice).

Time base setting shall be carried out with two reference echoes having a known time or distance interval between them. Depending on the intended calibration, the respective sound paths, depths, projection distances, or shortened projection distances shall be known.

This technique ensures that correction is automatically made for the sound propagation time through the delay block (e.g. probe wedge). Only in the case of equipment employing an electronically calibrated time base is one echo sufficient, provided the sound velocity of the reference block is known.

The distance between the reference echoes shall be as large as practicable within the time base range. The left-hand rising edge of each echo shall be set, using the time base shift and expansion controls, to correspond to a predetermined position along the horizontal screen graticule.

Where appropriate, calibration shall comprise a check signal, which shall not coincide with either one of the setting signals, but shall appear at the calculated screen position.

5.2 Reference blocks and reference reflectors

For the examination of ferritic steels the use of Calibration Block No.1 or Calibration Block No.2, as specified in EN 12223 and EN 27963 respectively, is recommended. If a reference block or the test object itself is used for calibration, faces opposite to the test surface or appropriate reflectors at different known sound path lengths may be used as applicable.

Either reference blocks shall have a sound velocity within $\pm 5\%$ of that of the test object, or correction for the velocity difference shall be made.

5.3 Straight beam probes

5.3.1 Single reflector technique

This requires a reference block having a thickness not greater than the time base range to be set. Suitable back wall echoes may be obtained from the 25 mm or 100 mm thickness of Calibration Block No. 1, or the 12,5 mm thickness of Calibration Block No. 2.

Alternative reference blocks, having parallel or concentric surfaces, known thickness, and the same sound velocity as the test object, may also be used.

5.3.2 Multiple reflector technique

This requires a reference block (or separate blocks) having two reflectors (e.g. side-drilled holes) at different known sound path lengths.

The probe shall be repeatedly repositioned to maximize the echo from each reflector; the position of the echo of the nearest reflector shall be adjusted using the shift (or zero) control and that of the echo of the other reflector using the expansion (or distance) control until an accurate time base setting is achieved.

5.4 Angle beam probes

5.4.1 Radius technique

Range setting can be performed using the radii reflectors of Calibration Block No. 1 or Calibration Block No. 2, as described in EN 12223 or EN 27963 respectively.

5.4.2 Straight beam probe technique

For transverse wave probes the range setting can be carried out using a longitudinal straight beam probe on the 91 mm thickness of Calibration Block No. 1 (described in EN 12223), corresponding to a sound path length of 50 mm for transverse waves in steel.

To complete the range setting it is necessary to obtain an echo, with the probe to be used for examination, from a suitable reflector at a known sound path distance, and using the zero shift control only, to position this echo at the correct location along the time base.

5.4.3 Reference block technique

This is similar in principle to that described in 5.3.2 for straight beam probes.

However to achieve adequate accuracy it is necessary to mark the beam index points on the surface of the block at which each echo is first maximized, and then mechanically measure the distance between these marks and the corresponding reflectors. For all subsequent time base adjustments, the probe shall be repositioned on these marks.

5.4.4 Contoured probes

Range setting shall first be performed using a probe with a flat face, as described above.

The contoured probe shall then be positioned on a suitable contoured reference block having at least one reflector at a known sound path length. The position of the echo from this reflector is adjusted to the correct position along the time base using only the shift control.

5.5 Alternative range settings for angle beam probes

5.5.1 Flat surfaces

Instead of setting in terms of sound path length, the time base may be set to indicate directly the depth of a reflector below the test surface, or its distance in front of the probe, see Figure 7.

Therefore, having selected the time base in terms of depth or projection distance, the echoes from the reference block, at known sound path lengths, are set along the time base at the positions corresponding to the equivalent depths, or projection distances, which may be determined as follows:

For a flat plate they may be determined for a given beam angle, either from a scale drawing, or from the following equations:

$$\text{- depth } (t): \quad t = s \cos \alpha_t \quad (8)$$

$$\text{- projection distance } (a): \quad a = s \sin \alpha_t \quad (9)$$

$$\text{- shortened projection distance } (a'): \quad a' = (s \sin \alpha_t) - x \quad (10)$$

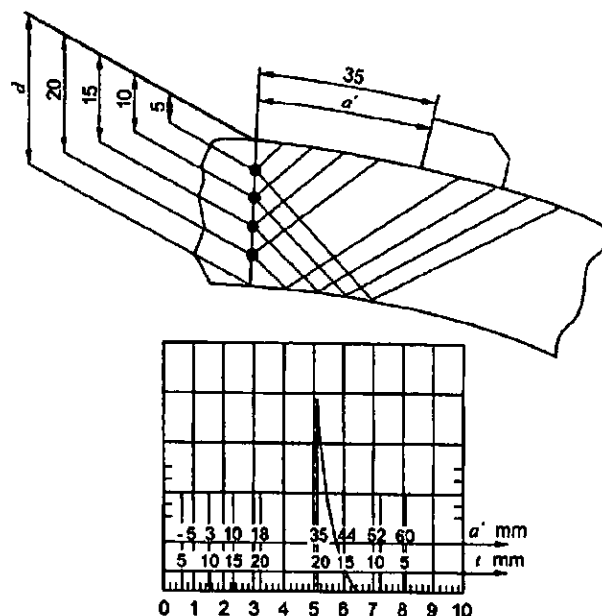


Figure 8 — Example of screen graticule for location of reflectors with a time base set in terms of reduced projection distance and depth (here: $\alpha_t = 51^\circ$, $s_{\max} = 100$ mm)

6 Sensitivity setting and echo height evaluation

6.1 General

After the time base has been calibrated, the sensitivity (or gain adjustment) of the ultrasonic equipment shall be set using one of the following techniques.

1) Single Reflector technique

A single reference reflector, e.g. a back wall, or a notch, may be used when evaluating echoes occurring within the same range of sound path distance.

2) Distance Amplitude Curve (DAC) technique

This technique uses the echo heights from a series of identical reflectors (e.g. side-drilled holes or flat-bottom holes) at different sound path lengths in suitable reference blocks (see 6.3).

3) Distance Gain Size (DGS) technique

This technique uses a series of theoretically derived curves relating the sound path length, the equipment gain, and the size of a disk-shaped reflector perpendicular to the beam axis (see 6.4).

Techniques 2 and 3 attempt to compensate for the change in the echo height from a reflector with increasing sound path distance. However, for all three techniques, a transfer correction shall be applied, where necessary, to compensate for any coupling losses and differences in material attenuation (see 6.5).

Using ideal reflectors of simple shape, e.g. side-drilled holes or flat bottom holes, for sizing of natural discontinuities, will not give the true size but only an equivalent value. The true size of the real discontinuity may be much larger than this equivalent value.

6.2 Angle of impingement

When using angle probes on curved test objects in conjunction with indirect scanning (i.e. after the $\frac{1}{2}$ skip position), the incident angle at the back wall, i.e. the angle of impingement, should be considered. In the case of cylindrical components scanned from the outer surface, the incident angle at the inner surface may be very much larger than the beam angle. Conversely, when scanning from the inner surface, the incident angle at the outer surface may be very much smaller than the beam angle (see annex C).

For transverse wave probes, the beam angle shall be chosen to avoid impingement angles outside the range 35° to 70° , because in that case severe loss in sound energy will occur due to mode conversion. Moreover, additional echoes from other wave modes may disturb echo evaluation.

A technique for determining the impingement angle at the inner and outer surfaces of a cylinder is described in annex C together with methods of calculating the sound path distance to the opposite surface.

6.3 Distance Amplitude Curve (DAC) technique

6.3.1 Reference blocks

A DAC reference block is required having a series of reflectors at different sound path distances over the time base range to be used for the test. Details of the spacing and minimum size of block and reflectors are given in annex B.

The specifications given in annex B apply for category 1 objects, and, where appropriate, for category 2 to category 5 test objects.

It should be noted that there are minimum sound path lengths below which signals cannot be satisfactorily evaluated due to e.g. dead zone effects or near field interference.

The DAC reference block shall be either:

- 1) a general purpose block of uniform low attenuation and specified surface finish, and having a thickness within $\pm 10\%$ of the test object; or
- 2) a block of the same acoustic properties, surface finish, shape and curvature as the test object.

In the case of type 1), correction for any differences in attenuation, curvature and coupling losses may be necessary before the Distance Amplitude Curve can be directly applied.

6.3.2 Preparation of a Distance Amplitude Curve

The distance amplitude curve shall be either shown directly on the screen of the instrument, or plotted on a separate graph, as described below. This may be supported by electronic means. When using equipment with Time Controlled Gain, TCG, (also known as 'Swept Gain',) gain will be controlled such that the DAC will become a straight horizontal line.

6.3.2.1 Plotting on screen

The time base is first calibrated to accommodate the maximum sound path length to be used, and the gain is adjusted so that the echoes from the series of reflectors fall within 20 % and 80 % of full screen height (FSH). In the case of angle probes, the reflectors may be used in either the 0 to $\frac{1}{2}$ skip, or $\frac{1}{2}$ to 1 skip positions.

The position of the tip of each maximized echo, at a constant gain setting, is then marked on the screen, and the Distance Amplitude Curve drawn through the points.

If the difference in height between the largest and smallest echoes exceeds the range 20 % to 80 % FSH, the line shall be split, and separate curves plotted at different gain settings (see Figure 9). The difference in gain between the two curves shall be recorded on the screen.

The gain setting used for plotting the DAC may be referenced to the echo from some other reflector, e.g. in the case of flat probes to either the 100 mm radius quadrant, or the 3 mm diameter hole in Calibration Block No. 1. This will enable the gain to be reset, in future, without the use of the reference block.

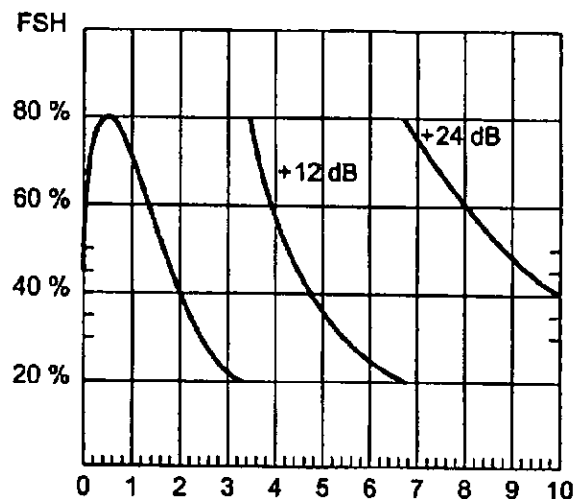


Figure 9 — Screen of ultrasonic instrument showing a split Distance Amplitude Curve (DAC)

6.3.2.2 Plotting on a separate graph

The general procedure is similar to technique 6.3.2.1 except that the maximized echo from each reflector is adjusted to the same height (generally 80 % FSH) and the gain setting noted and plotted against the sound path length on a separate graph.

6.3.2.3 Transfer correction

After determining transfer differences using the data obtained under 6.5, the Distance Amplitude Curve, as produced to 6.3.2.1 and 6.3.2.2, shall be corrected accordingly.

This may be achieved by either:

- 1) correcting the DAC during its preparation;
- 2) drawing a second, corrected, DAC;
- 3) applying appropriate correction values in the evaluation process.

While techniques 1 and 2 may be preferable if a sound path dependent attenuation correction is needed, technique 3 may be more suitable in cases where allowance is required only for a constant transfer correction.

6.3.3 Evaluation of signals using a Distance Amplitude Curve

6.3.3.1 Setting the test sensitivity

The test sensitivity shall be set by maximizing the echo from one of the reference reflectors in the DAC reference block and adjusting the gain to bring the peak of the echo up to the DAC.

The gain shall then be increased by the transfer correction at the appropriate sound path length, if it has not been incorporated in the DAC itself (methods 1 and 2 above).

Alternatively, if the gain setting for the Distance Amplitude Curve has been referenced to another reflector, this may be used instead, using the appropriate gain correction.

The gain is then increased (or decreased) prior to scanning by the value specified in the relevant standard or procedure.

6.3.3.2 Measurement of echo height

The height of any echo, which requires to be evaluated, is adjusted using the calibrated gain control, to bring it to the DAC, and recorded in terms of the increase or decrease in gain setting compared to the original value at which the DAC was plotted. If not already incorporated in the DAC, appropriate values for transfer correction shall be added if necessary.

Evaluation of the resulting echo height difference is as follows:

Where the gain setting has required to be increased from the original value by x dB, the echo height is assigned a value (reference level $- x$)dB. Where the gain setting has required to be decreased from the original value by y dB, the echo height is assigned a value (reference level $+ y$)dB.

6.3.4 Evaluation of signals using a reference height

In this method the discontinuity echo is compared to the echo from a reference reflector having the same or larger sound path length. The two signals are set to equal screen height (i.e. the reference height), using gain settings V_u and V_r , respectively. The reference height shall be within 40 % and 90 % FSH. The echo height difference, ΔH_u , shall then be calculated using equation 11:

$$\Delta H_u = V_r - V_u \quad (11)$$

6.4 Distance Gain Size (DGS) technique

6.4.1 General


The DGS technique uses the theoretically derived distance amplitude curves of disk-shaped reflectors to evaluate the echo height of unknown reflectors.

In the general DGS diagram, distance and reflector size are normalized. Therefore, it is independent of probe (element) size and frequency. It shows distance as multiples of the near field length N_{eff} of the probe, and reflector sizes as multiples of the probe element diameter D_{eff} (see Figure 10 and annex D).

From this general DGS diagram, special DGS diagrams for common types of probes are derived for steel, which allow the direct reading of equivalent reflector size without calculation (see Figure 11).

The echo height from a reflector is recorded in terms of either:


- i) the number of dB above or below the DGS curve for a specified reflector diameter; or
- ii) the diameter of a disk-shaped reflector that would give the same echo height under ideal conditions and at the same sound path distance (equivalent disc).

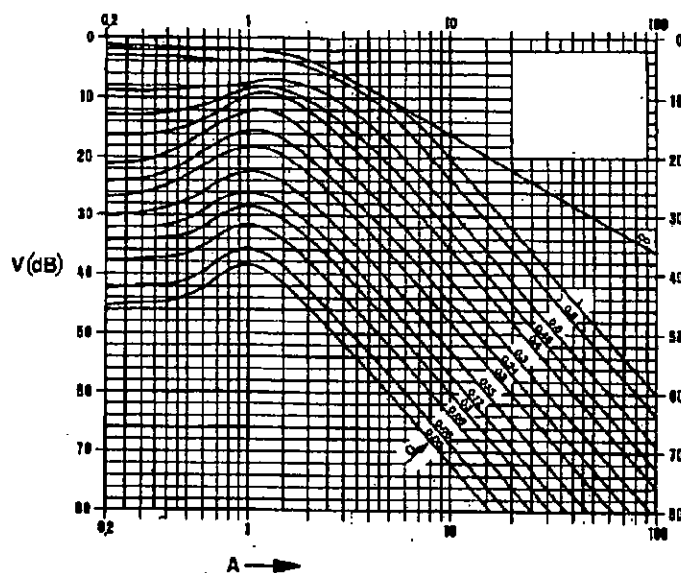

Key

A normalized distance
 V gain in dB
 G normalized reflector size

Figure 10 — General DGS diagram

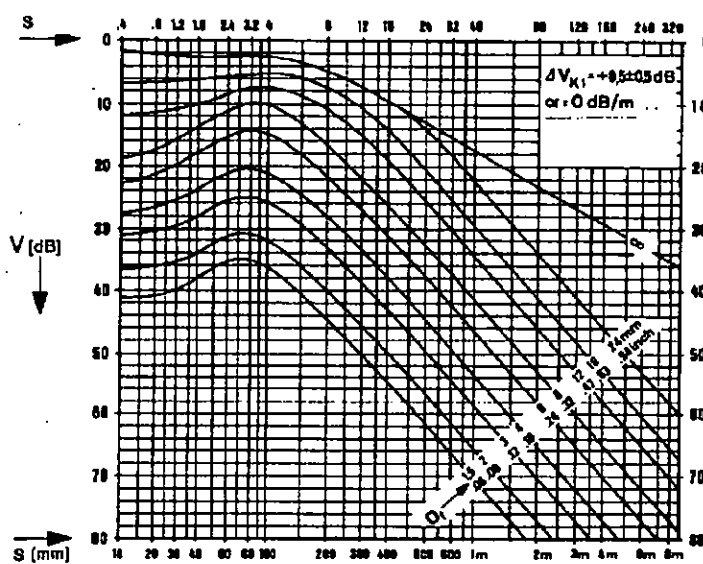

Key

s reflector distance
 V gain in dB
 D_r reflector diameter

Figure 11 — Specific DGS diagram for an angle beam probe on steel

6.4.2 Reference blocks

When using the DGS technique for setting the test sensitivity, or recording echo height, an applicable reference block, as specified in annex B, shall be employed. This is in order to relate the gain values shown in the DGS diagram to the echo height from a suitable reference reflector. The test block may possibly be used as the reference block.

Reference blocks for angle probes shall be large enough to permit the through-transmission measurements to be made necessary for determining transfer loss. All test surfaces of the reference blocks shall have the same finish.

Concave cylindrical surfaces (e.g. the quadrants of Calibration Block No. 1 and Calibration Block No. 2 as specified in EN 12223 or in EN 27963) shall be employed for the calibration of sensitivity by the DGS method, only if the probe specific correction factor, ΔV_k , for these blocks is known. This is in order that compensation can be made for the difference in reflection of the quadrant compared to that of a plane back wall. If the sign of ΔV_k is positive it means that the gain for the examination has to be increased by that value and vice versa.

To prevent total reflection of the sound beam at the surface of a curved reference block, or test object, the diameter of curvature, D_{obj} , shall fulfil the following condition:

$$D_{obj} > D_{eff} \left(\frac{c_t}{c_d} \times \frac{1}{1 - \sin \alpha_t} \right) \quad (12)$$

where:

- D_{eff} is the effective diameter of the transducer;
- c_t is the sound velocity of transverse wave in test object;
- c_d is the longitudinal wave velocity in delay block;
- α_t is the beam angle.

As an example, the value of D_{obj} (steel) shall be greater than 82 mm for a 45° angle beam probe with an effective transducer diameter of 20 mm.

6.4.3 Use of DGS diagrams

6.4.3.1 Reference height technique

The recording gain V_r , at which scanning shall be carried out, is calculated from equation 13:

$$V_r = V_j + \Delta V + \Delta V_k + \Delta V_t \quad (13)$$

where:

V_j is the gain setting required to set the echo from a reference reflector, meeting the requirements of annex B, to a given reference height on the screen (not less than 20 % FSH);


ΔV is the difference in gain between the DGS curve corresponding to the minimum equivalent disk-shaped reflector (i. e. the recording level), measured at the maximum sound path length s_{max} , and the reference reflector, measured at its sound path length s_j ;

ΔV_k is a correction factor when using a concave reference reflector (see 6.4.2);

ΔV_t is the transfer correction (see 6.5).

The height of any echo observed during scanning which meets or exceeds the reference height on the screen, shall be assessed as follows:

The gain V_u necessary to bring the echo to the reference height shall be noted. A line representing the reference height shall then be drawn on the DGS diagram, and the gain difference $\Delta V_u = V_u - V_r$ marked off from the reference height at the corresponding sound path distance, s_u (see Figure 12). If the marked point is above the DGS curve associated with the recording limit, the echo height ΔH_u shall be recorded in terms of the number of dB by which it exceeds the DGS curve at the same sound path distance.

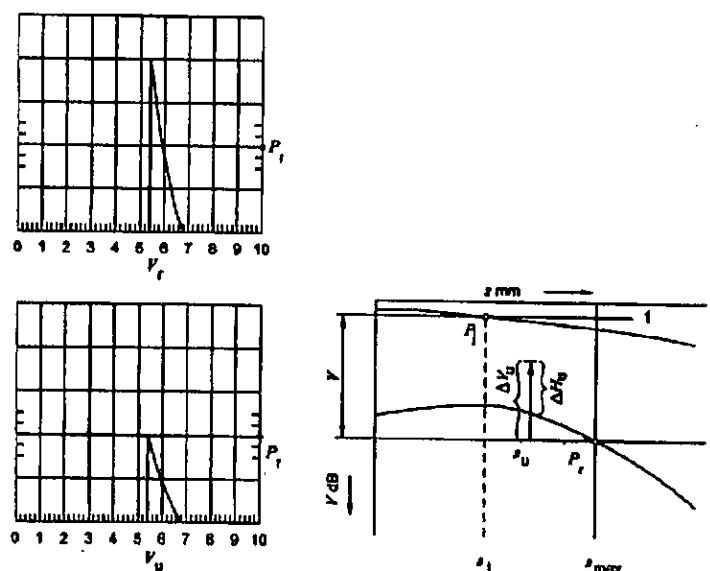

Key

- 1 calibration height
- 2 reference height
- 3 reference line

Figure 12 — Example of echo height evaluation using the reference height technique

6.4.3.2 Reference line technique

The curve on the DGS diagram, associated with the recording limit, shall be transferred as a reference line from the DGS diagram to the screen. Note that the relationship between the difference in gain of the DGS diagram (ΔV) at different sound paths is a logarithmic one, whereas the corresponding scaling on the screen is linear:

$$\Delta V \text{ (in dB)} = -20 \log_{10} \left(\frac{h_1}{h_2} \right) \quad (14)$$

where h_1 and h_2 are the actual physical screen heights, e.g. expressed as a percentage full screen height (FSH).

The difference in gain (ΔV) between the echo from the reference reflector and the DGS curve corresponding to the recording limit, at the same sound path distance, is measured on the DGS diagram.

The echo from the reference reflector is then maximized, and the gain adjusted to set the tip of the echo to a convenient height on the screen (see below).

This position is marked, and the transferred DGS curve drawn through it. The reference line shall be between 20 % and 80 % full screen height. To achieve this, the reference line and recording gain may be raised or lowered within a particular section, as shown in Figure 9.

The gain is then changed for scanning by ΔV and by the possible corrections as given in 6.4.3.1.

The height of any echo observed during scanning, equal to or exceeding the corrected DGS curve, shall be recorded in terms of either:

- a) the number of dBs that it exceeds the corrected DGS curve by at the same sound path distance;
- b) the equivalent disk-shaped reflector diameter, shown on the DGS diagram, that corresponds to the difference in echo height measured in (a) above.

6.4.4 Restrictions on use of the DGS technique due to geometry

Echo height evaluation using the DGS method is only applicable if contouring of the probe shoe is not required, see 3.4.

The conditions given in annex B for reference blocks, shall also apply to the relevant surfaces of the test object. For echo height evaluation, the following condition for the normalized distance A shall be satisfied (see annex D for the calculation of A):

$$A \geq 0,7 \quad (15)$$

With regard to the wall thickness d , conditions (16) and (17) shall also be satisfied for straight beam scanning without delay path, and for angle beam scanning respectively:

$$d > 0,7 N_{\text{eff}} \quad (N_{\text{eff}} \text{ is the effective near field length}) \quad (16)$$

$$d > 5 \lambda \quad (\lambda \text{ is the wavelength in the test object}) \quad (17)$$

6.5 Transfer correction

6.5.1 General

Unless the test sensitivity is set on a test block which is acoustically representative of the test object, a transfer correction shall be determined, and applied if necessary, when setting the test sensitivity or measuring the echo height of any discontinuity.

The transfer correction ΔV_t is made up of two parameters:

- 1) one due to coupling losses at the contact surface and independent of sound path length;
- 2) one due to material attenuation and dependent on sound path length.

Two methods are described, namely: a simple fixed path length method where compensation is made for coupling loss, and for attenuation at the maximum sound path length only; and a comparative method where full compensation is made for both parameters.

6.5.2 Fixed path length technique

This technique is only applicable where either the loss in acoustic energy due to attenuation is small compared to the coupling loss, or the reflector, whose echo height is to be measured, lies close to the back-wall of the test object.

When using a straight beam probe, the gain values required to bring the first back-wall echoes from the reference block and the test object to the same height on the screen are measured in dB ($V_{t,t}$ and $V_{t,r}$ respectively). When using an angle beam probe, two identical probes are employed as separate transmitter and receiver in V-formation to produce the corresponding echoes.

The theoretical difference in gain between the two echoes (ΔV_s), due to their different sound path lengths, shall be measured on the DGS curve for an infinite reflector, and the transfer correction (ΔV_t) calculated as follows:

$$\Delta V_t = V_{t,t} - V_{t,r} - \Delta V_s \quad (18)$$

6.5.3 Comparative technique

6.5.3.1 Straight beam probe

The probe is placed on the reference block and the gain settings required to bring the first and second back-wall echoes up to the same height on the screen are recorded (values V_{A1} , V_{A2} in Figure 13). These values are then plotted against sound path length, and a line (2) drawn through them.

The probe is then repositioned on the test object and the above procedure repeated (values V_{B1} and V_{B2} and line 1 in Figure 13).

The transfer correction (ΔV_t) at the appropriate sound path length (s_u) is given by the difference in gain between the two lines, see Figure 13.

Note that the slope of the line plotted through V_{B1} and V_{B2} does not give the true attenuation in the test object, since no account is taken of the losses caused by beam divergence and the energy transmitted into the probe at each multiple reflection at the examination surface. Annex E gives a method to experimentally determine those contact transfer losses at each multiple reflection.


6.5.3.2 Angle beam probe

The technique is similar in principle to that for straight beam probes, except that two identical angle beam probes, operating as separate transmitter and receiver, are used. The frequency of these probes shall be the same as that of the probe(s) to be used for the examination of the test object.

The probes are positioned on the DAC reference block, first in V-formation, and then in W-formation, and the gain settings required to bring the echoes to the same height on the screen are recorded (values V_{A1} and V_{A2} respectively). The probes are then similarly positioned on the test object, and the procedure repeated (values V_{B1} and V_{B2}).

The recorded gain values are plotted against the sound path length, and lines drawn through each pair of points.

The transfer correction, ΔV_t , is again given by the difference in gain between the two lines at the appropriate sound path length.

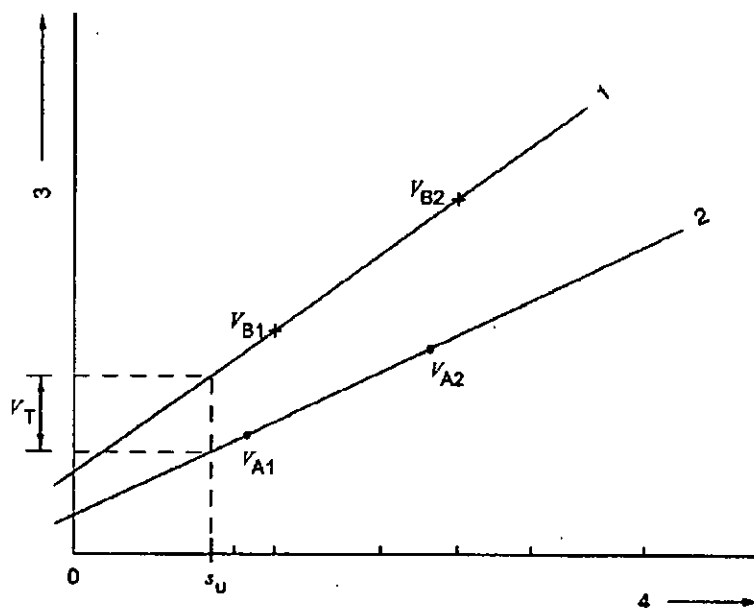

Key

- 1 curve for test object
- 2 curve for reference block
- 3 gain setting for 80 % FSH
- 4 sound path length

Figure 13 — Determination of transfer correction using the comparative method

6.5.4 Compensation for local variations in transfer correction

If there is reason to suspect local variations in transfer correction over the area of the object to be examined, the transfer correction shall be measured at a number of representative positions.

If the variation in transfer correction between the upper and lower values does not exceed 6 dB, the value to be employed shall be the average, ΔV_t , of all the measurements made. If, however, the above variation is greater than 6 dB, methods (a) or (b) below shall be applied:

- a) Increase the average transfer correction, ΔV_t , by a value equal to the average, ΔV_{\sim} , of all the measurements above ΔV_t . The revised transfer correction ($\Delta V_t + \Delta V_{\sim}$), shall be applied over the whole of the area to be examined;
- b) divide the area to be examined into zones, such that within each zone the variation in transfer correction does not exceed 6 dB. A separate value of ΔV_t shall then be applied to each zone.

For oblique scanning, through transmission signals shall be employed instead of back-wall echoes.

Annex A
(normative)

Table A.1 — Quantities and symbols

Symbol	Quantity	Unit
A	Normalized distance in DGS diagram	
A'	Probe co-ordinate	mm
a	Projection distance	mm
a'	Reduced projection distance	mm
α	Measured beam angle in steel	°
α_r	Beam angle in a non-alloy steel reference block	°
α_d	Incident angle (beam angle in delay block)	°
α_t	Beam angle in test object	°
β	Angle of impingement	°
c_r	Sound velocity in reference block	m/s
c_t	Velocity of transverse sound wave in test object	m/s
c_d	Velocity of longitudinal sound wave in delay block	m/s
D_{obj}	Outer diameter of test object or curvature of scanning surface	mm
d	Wall thickness	mm
D_{eff}	Effective diameter of transducer	mm
D_{SSH}	Diameter of hole with spherical bottom	mm
D_{DSR}	Diameter of disk-shaped reflector	mm
D_P	Probe diameter	mm
D_{SDH}	Diameter of side-drilled hole	mm
e_1 to e_7	Reference block dimensions	mm
g	Depth of contour on probe face	mm
G	Normalized diameter of disk-shaped reflector in DGS diagram	
λ	Wavelength	mm
ΔH_u	Echo height difference between a reference reflector and a discontinuity	dB
l_{ps}	Length of probe shoe in direction of curvature	mm
l_d	Length of delay path	mm
Δl_{ps}	Length of contoured probe face	mm
N_{eff}	Effective near field length	mm
P_r	Reference point at s_{max}	
P_j	Reference point at s_j	
q	Transverse co-ordinate of reflector	mm
s	Sound path length	mm

Table A.1 (continued)

Symbol	Quantity	Unit
s_j	Sound path length of reference reflector	mm
s_{max}	Maximum sound path length	mm
s_u	Sound path length associated with evaluated signal	mm
s_v	Acoustic equivalent to delay path in test object	mm
l	Depth co-ordinate of reflector	mm
V	Gain in DGS diagram	dB
V_j	Calibration basic gain	dB
V_t	Recording gain	dB
V_l	Gain for determining ΔV_t	dB
V_u	Indication gain	dB
ΔV	Gain difference	dB
ΔV_c	Correction for ΔV_t	dB
ΔV_k	Gain correction for concave reflector	dB
ΔV_s	Gain difference associated with sound path length	dB
ΔV_t	Transfer correction (average)	dB
$V_{l,r}$	Gain for back-wall echo on reference block	dB
$V_{l,t}$	Gain for back-wall echo on test object	dB
ΔV_u	Difference between indication gain and recording gain	dB
w_{ps}	Width of probe shoe in direction of curvature	mm
Δw_{ps}	Width of contouring of the probe face	mm
x	Distance between probe index and front edge of probe, for uncounted probe	mm
Δx	Probe index shift	mm

Annex B
(normative)

Reference blocks and reference reflectors

Table B.1 — Reference Blocks. Requirements for scanning surface, wall thickness, and back wall

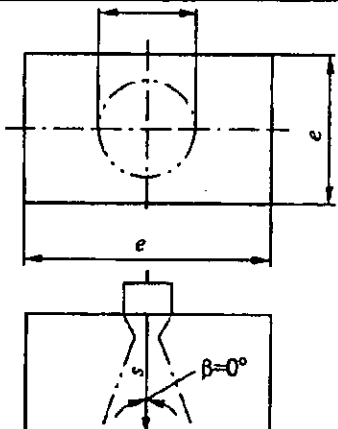
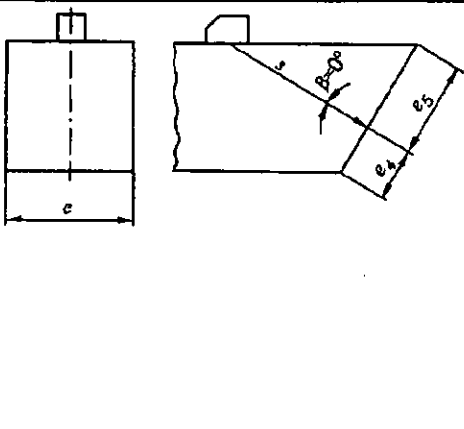
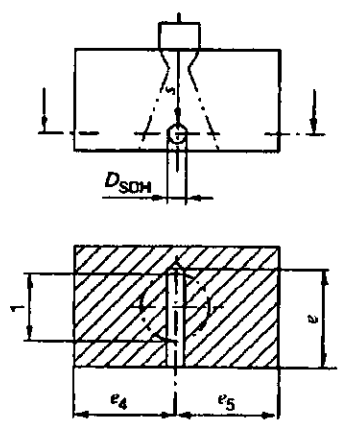
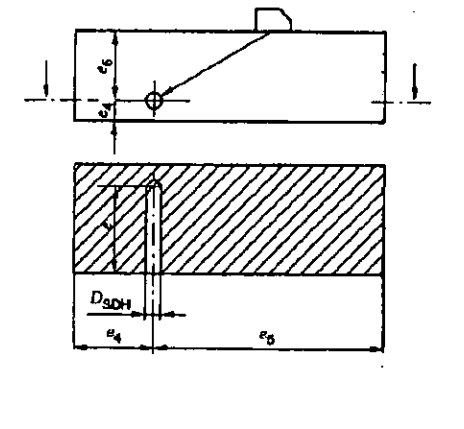
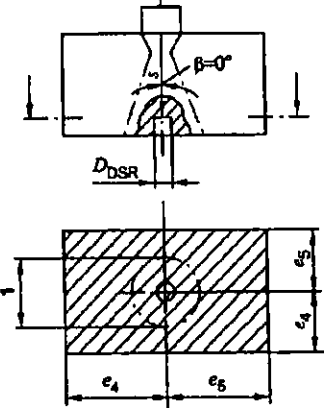
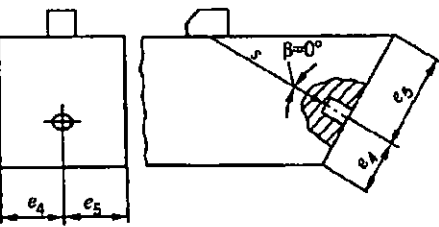
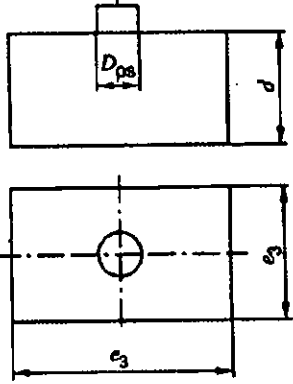
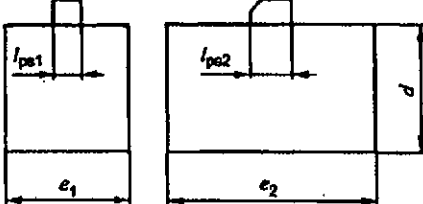
Requirements to be met by back wall examination using:		
normal probe	angle probe	condition
 <p>Key</p> <p>1 Sound beam diameter</p>		$e > \frac{2\lambda s}{D_{\text{eff}}}$ $e_4, e_5 > \frac{\lambda s}{D_{\text{eff}}}$
Requirements to be met by side-drilled hole for examination using:		
Normal probe	angle probe	condition
 <p>Key</p> <p>1 Sound beam diameter</p>		$D_{\text{SDH}} \geq 1,5\lambda$ $e > \frac{2\lambda s}{D_{\text{eff}}}$ $e_4, e_5 > \frac{\lambda s}{D_{\text{eff}}}$ $s > 1,5 N_{\text{eff}} \text{ with}$ $D_{\text{DSR}} = \sqrt{\frac{\sqrt{2}}{\pi}} \lambda \sqrt{s D_{\text{SDH}}}$

Table B.1 (continued)

Requirements to be met by disk-shaped reflector for examination using:		
normal probe	angle probe	conditions
		$D_{DSR} < \frac{\lambda s}{D_{eff}}$ $e_4, e_5 > \frac{\lambda s}{D_{eff}}$ $s > 0,7 N_{eff}$
Key 1 sound beam diameter		

Requirements to be met by test surface and wall thickness for examination using:		
normal probe	angle probe	condition
		<p>d larger than the length of the initial pulse influence zone for α equal to 0°.</p> $d > 5 \lambda \text{ for } \alpha > 0^\circ.$ $e_1 > 1,5 I_{ps1}$ $e_2 > 1,5 I_{ps2}$ $e_3 > 1,5 D_{ps}$


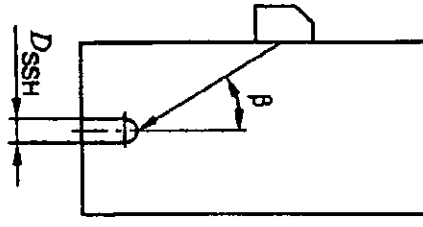
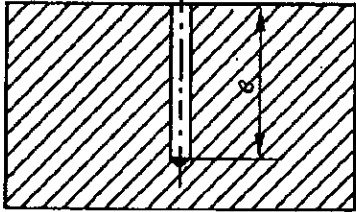
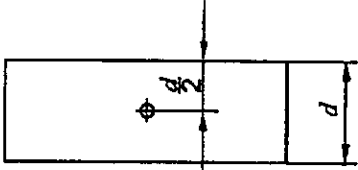
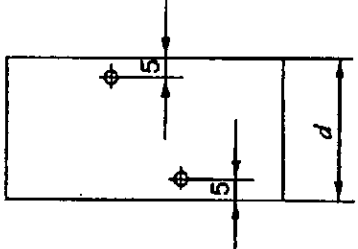
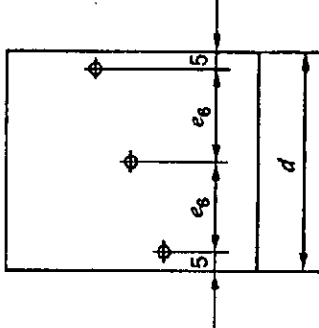
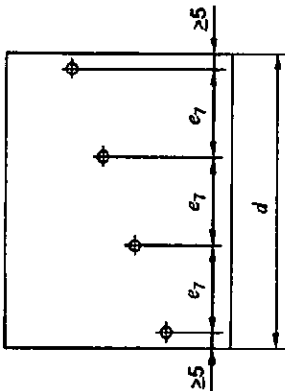
Requirements to be met by holes with spherical bottom for examination using		
normal probe	angle probe	conditions
		$s > 1,5 N_{eff} \text{ with}$ $D_{DSR} = \sqrt{\frac{\lambda}{\pi}} D_{SSH}$ $\beta \leq 60^\circ.$ $e_4, e_5 > \frac{\lambda s}{D_{eff}}$

Table B.2 — Reference blocks and reference reflectors for class 1 objects

Wall thickness, d , in mm	Reference blocks and reference reflectors	Conditions
		
$10 \leq d \leq 15$		
$15 < d \leq 20$		$e > \frac{2\lambda s}{D_{\text{eff}}}$
$20 < d \leq 40$		$D_{\text{SDH}} \geq 1,5\lambda$ $e_6 = \frac{d-10}{2}$
$d > 40$		$e_7 \leq \frac{d-10}{2}$

Annex C (normative)

Determination of sound path distance and impingement angle in concentrically curved objects

C.1 Impingement angle

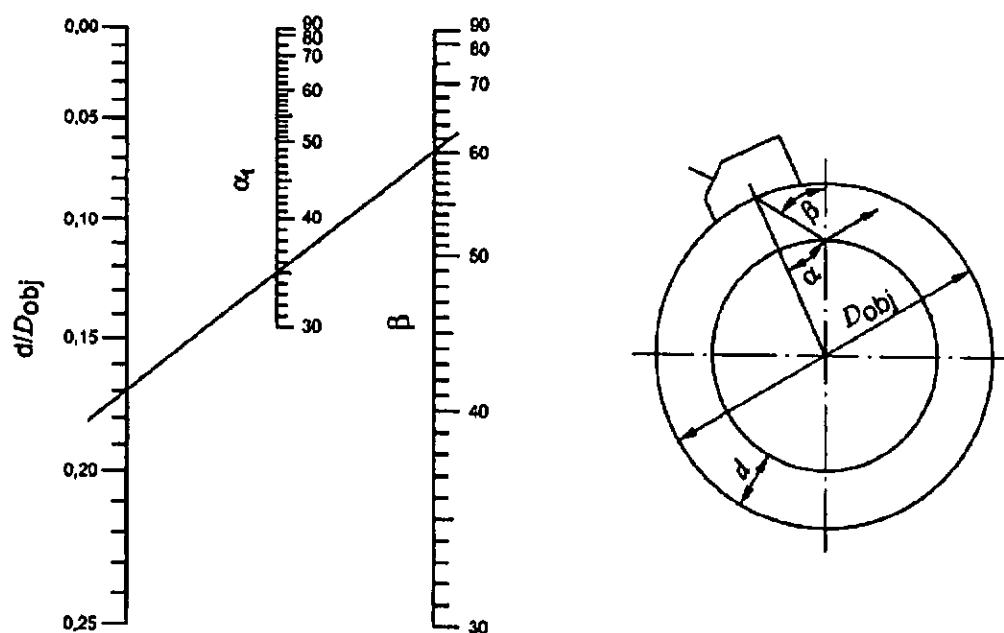


Figure C.1— Nomogram for determination of impingement angle, β

C.2 Sound path when scanning from the outer (convex) surface:

$$s = (D_{\text{obj}} \cos \alpha) - \sqrt{(D_{\text{obj}} \cos \alpha)^2 - 4d(D_{\text{obj}} - d)} \quad (\text{C.1})$$

C.2.1 Full skip

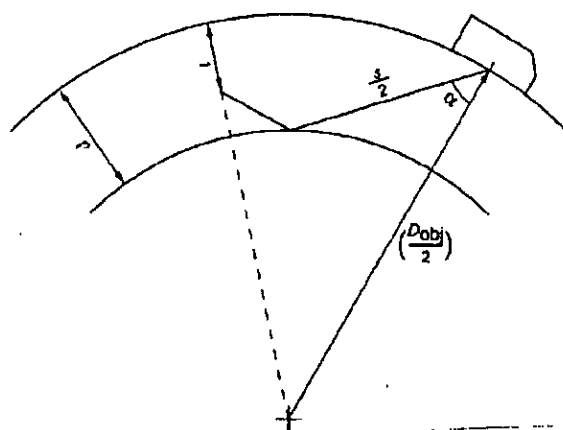


Figure C.2 — Determination of sound path distance for scanning from the outer surface in full skip

$$s_t = \left[1 - \left(\frac{t}{2d} \right) \right] \left[(D_{\text{obj}} \cos \alpha) - \sqrt{(D_{\text{obj}} \cos \alpha)^2 - 4d(D_{\text{obj}} - d)} \right] \quad (\text{C.2})$$

where s_t is the total sound path.

C.2.2 Half skip

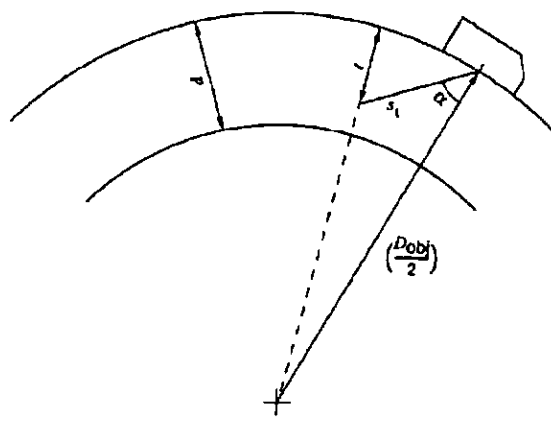


Figure C.3 — Determination of sound path distance for scanning from the outer surface in half skip

$$s_t = \left(\frac{t}{2d} \right) \left[(D_{\text{obj}} \cos \alpha) - \sqrt{(D_{\text{obj}} \cos \alpha)^2 - 4d(D_{\text{obj}} - d)} \right] \quad (\text{C.3})$$

where s_t is the total sound path.

C.3 Soundpath when scanning from the inner (concave) surface:

$$s = -2 \left\{ \left(\frac{D_{obj}}{2} - d \right) \cos \alpha - \sqrt{\left[\left(\frac{D_{obj}}{2} - d \right) \cos \alpha \right]^2 + d(D_{obj} - d)} \right\} \quad (C.4)$$

C.3.1 Full skip

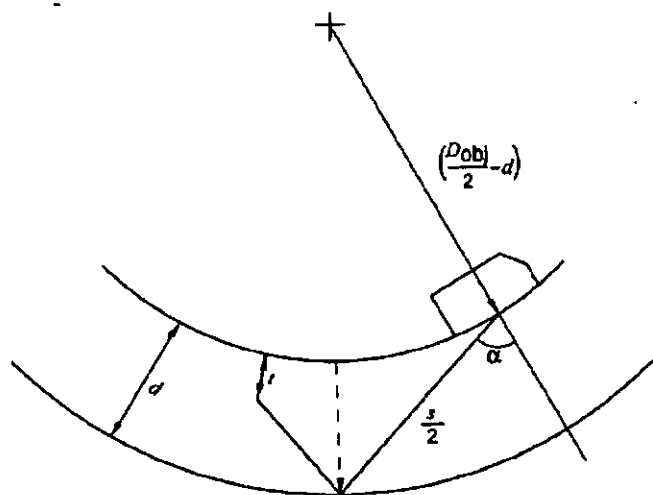


Figure C.4 — Determination of sound path distance for scanning from the inner surface in full skip

$$s_t = -2 \left\{ \left[1 - \left(\frac{t}{2d} \right) \right] \left[\left(\frac{D_{obj}}{2} - d \right) \cos \alpha - \sqrt{\left[\left(\frac{D_{obj}}{2} - d \right) \cos \alpha \right]^2 + d(D_{obj} - d)} \right] \right\} \quad (C.5)$$

where s_t is the total sound path.

C.3.2 Half skip

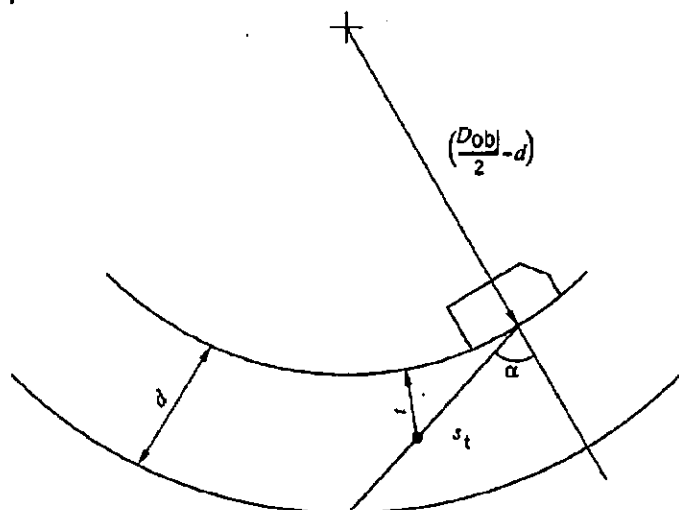


Figure C.5 — Determination of sound path distance for scanning from the inner surface in half skip

$$s_t = \left(\frac{t}{d} \right) \left[\left(\frac{D_{obj}}{2} - d \right) \cos \alpha - \sqrt{\left(\left(\frac{D_{obj}}{2} - d \right) \cos \alpha \right)^2 + d(D_{obj} - d)} \right] \quad (C.6)$$

where s_t is the total sound path.

Annex D (informative)

General DGS diagram

This is a theoretically derived diagram applicable to all single transducer, straight or angle beam probes having a known natural focus (effective near field length N_{eff}). It expresses the relationship between echo height or gain (in dB), and the sound path distance expressed in near field lengths for the probe in use, for a series of disk-shaped reflectors. The size of the reflectors is expressed in terms of the effective transducer diameter D_{eff} of the probe in use. The general DGS diagram is shown in Figure 10.

D.1 Distance

The normalized distance, A , is given by the equation:

$$A = \frac{s + s_d}{N_{\text{eff}}} \quad (\text{D.1})$$

and

$$s_d = l_d \left(\frac{c_d}{c_t} \right) \quad (\text{D.2})$$

where:

- s is the sound path distance to reflector;
- s_d is the equivalent sound path distance in the delay block of the probe;
- N_{eff} is the near field length of probe in test object;
- l_d is the length of delay path;
- c_d is the longitudinal wave velocity in delay block;
- c_t is the wave velocity in test object.

For straight beam probes without a delay block the equation simplifies to:

$$A = \frac{s}{N_{\text{eff}}} \quad (\text{D.3})$$

D.2 Gain

The gain, V , is the logarithmic value of the ratio between echo height on the screen ($[H_R]_{A \rightarrow 0}$) for a large planar reflector (e.g. back-wall) situated immediately in front of the transducer, and the echo height ($[H_{\text{DSR}}]_A$) of a disk-shaped reflector at distance A .

$$V = -20 \log_{10} \left(\frac{[H_R]_{A \rightarrow 0}}{[H_{\text{DSR}}]_A} \right) \quad (\text{D.4})$$

In general, the gain difference, ΔV , between two echoes is determined by noting the change in gain setting of the instrument necessary to bring both echoes to the same height on the screen.

D.3 Size

The normalized size, G , of a reflector is expressed in terms of the ratio of the actual diameter of a disk-shaped reflector, D_{DSR} , to that of the effective transducer diameter, D_{eff} , of the probe in use.

$$G = \frac{D_{\text{DSR}}}{D_{\text{eff}}} \quad (\text{D.5})$$

Annex E (informative)

Determination of contact transfer correction factors

E.1 General

As usual the gain V in decibels is given by:

$$V = -20 \log_{10}(A/A_0) \quad (\text{E.1})$$

where A and A_0 are signal amplitudes.

During propagation a sound wave suffers from three different losses:

- Divergence losses V_D caused by the probe and the material.
With distance the sound pressure decreases. Curves are shown e.g. in the DGS diagram (Figure 10);
- Attenuation losses V_A caused by the material of the test object (absorption and scattering).
Usually sound pressure decreases with distance following an exponential function;
- Contact transfer losses V_{CT} caused by the contact matching of the probe to the test object via a coupling fluid.
Every time the reflected sound wave passes this area, part of the energy enters the probe and the other part is reflected back for further multiple echoes (see Figure E.1).

E.2 Measurement

To measure these contact transfer losses, which are not constant but depending on distance, the divergence losses V_D and attenuation losses V_A have to be eliminated.

To keep these losses V_A and V_D constant during the measurement, a set of at least three plane parallel plates made of the same material are used with the same probe under constant coupling conditions (fluid, load, rest time, temperature). The thicknesses t_1 , t_2 , t_3 of these plates have the ratios $t_3 = 2t_2 = 4t_1$.

Using plate 1 with thickness t_1 , four echoes are generated with the amplitudes $V1(t_1)$, $V1(2t_1)$, $V1(3t_1)$, $V1(4t_1)$, which are noted.

Similarly, plate 2 with thickness t_2 gives two echoes with the amplitudes $V2(t_2)$, $V2(2t_2)$.

Finally, the first echo from plate 3 with thickness t_3 gives an amplitude $V3(t_3)$.

E.3 Evaluation

The second echo from plate 2 with thickness t_2 and the first echo from plate 3 with thickness t_3 have the same sound path length, therefore their losses V_A and V_D are equal.

The difference of their dB-readings give the contact transfer loss at distance t_2 :

$$V2(2t_2) - V3(t_3) = V_{\alpha}(t_2) \quad (\text{E.2})$$

The second echo from plate 1 with thickness t_1 and the first echo from plate 2 with thickness t_2 , give the contact transfer loss at distance t_1 :

$$V1(2t_1) - V2(t_2) = V_{\alpha}(t_1) \quad (\text{E.3})$$

The fourth echo from plate 1 with thickness t_1 and the first echo from plate 3 with thickness t_3 have also equal losses V_A and V_D , but the measured value $V1(4t_1)$ includes the contact transfer losses at three different distances: t_1 , $2t_1$, $3t_1$.

The losses at t_1 and $2t_1 = t_2$ have already been determined by equations (E2) and (E3). So the unknown loss $V_{\alpha}(3t_1)$ can be calculated by:

$$V1(4t_1) - V3(t_3) - V_{\alpha}(t_1) - V_{\alpha}(t_2) = V_{\alpha}(3t_1) \quad (\text{E.4})$$

With these three values for the contact transfer losses at three different distances, a graph can be plotted as Figure E.2 shows.

Contact transfer losses for all distances between $0,5t_1$ and $3,5t_1$ can be read off the diagram without further measurement.

They are only valid for the used combination of probe, coupling fluid and material.


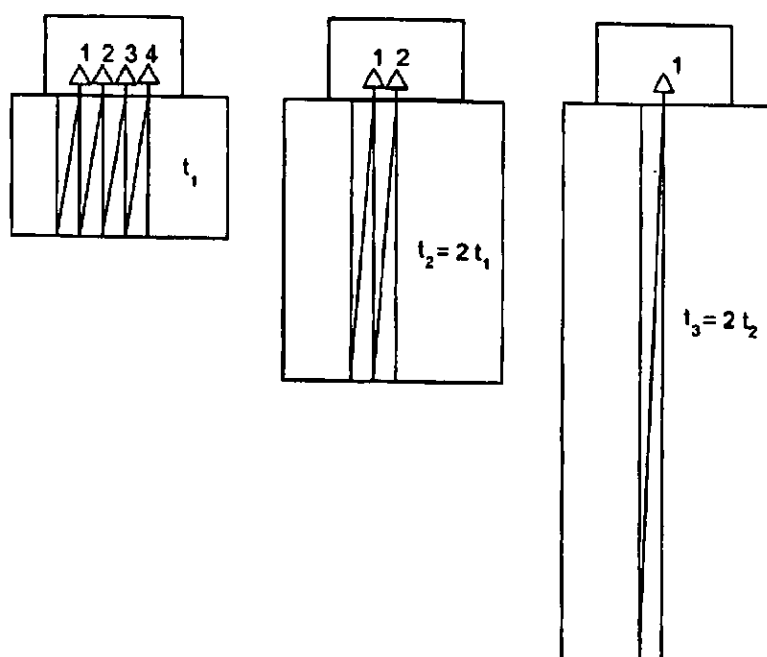


Figure E.1 — Setup for determination of contact transfer losses

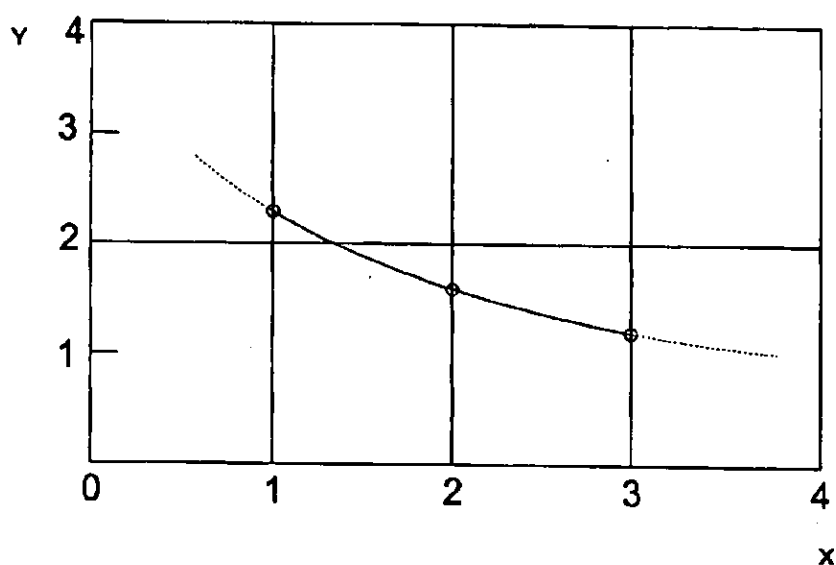

Key

y contact transfer loss V_{ct} in dB
 x sound path distance in multiples of t_1

Figure E.2 — Determination of contact transfer losses

Bibliography

- prEN 583-4:1999, *Non-destructive testing — Ultrasonic examination —
Part 4: Examination for discontinuities perpendicular to the surface.*
- ENV 583-6, *Non-destructive testing — Ultrasonic examination —
Part 6: Time-of-Flight Diffraction Technique as a method for detection
and sizing of discontinuities.*

BS EN
583-2:2001

BSI — British Standards Institution

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

Revisions

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover.
Tel: 020 8996 9000. Fax: 020 8996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

Buying standards

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services. Tel: 020 8996 9001. Fax: 020 8996 7001. Standards are also available from the BSI website at <http://www.bsi-global.com>.

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

Information on standards

BSI provides a wide range of information on national, European and international standards through its Library and its Technical Help to Exporters Service. Various BSI electronic information services are also available which give details on all its products and services. Contact the Information Centre.
Tel: 020 8996 7111. Fax: 020 8996 7048.

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration.
Tel: 020 8996 7002. Fax: 020 8996 7001. Further information about BSI is available on the BSI website at <http://www.bsi-global.com>.

Copyright

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

If permission is granted, the terms may include royalty payments or a licensing agreement. Details and advice can be obtained from the Copyright Manager.
Tel: 020 8996 7070.

BSI
389 Chiswick High Road
London
W4 4AL