

Chemical analysis of ferrous materials — Determination of total carbon in steels and irons — Gravimetric method after combustion in a stream of oxygen

This European Standard EN 10036:1989 has the status of a
British Standard

Cooperating organizations

The European Committee for Standardization, under whose supervision this European Standard was prepared, comprises the national standards organizations of the following Western European countries.

Austria	Oesterreichisches Normungsinstitut
Belgium	Institut belge de normalisation
Denmark	Dansk Standardiseringsraad
Finland	Suomen Standardisoimisliitto, r.y.
France	Association française de normalisation
Germany	Deutsches Institut für Normung e.V.
Greece	Hellenic Organization for Standardization
Iceland	Technological Institute of Iceland
Ireland	National Standards Authority of Ireland
Italy	Ente Nazionale Italiano di Unificazione
Luxemburg	Inspection du Travail et des Mines
Netherlands	Nederlands Normalisatie-instituut
Norway	Norges Standardiseringsforbund
Portugal	Instituto Português da Qualidade
Spain	Asociación Española de Normalización y Certificación
Sweden	Standardiseringskommissionen i Sverige
Switzerland	Association suisse de normalisation
United Kingdom	British Standards Institution

This British Standard was published under the authority of the Board of BSI and comes into effect on 31 January 1991

© BSI 12-1999

The following BSI references relate to the work on this standard:
Committee reference ISM/18
Draft for approval 83/70400

ISBN 0 580 19305 5

Amendments issued since publication

Amd. No.	Date of issue	Comments

Contents

	Page
Cooperating organizations	Inside front cover
National foreword	ii
Brief history	2
Text of EN 10036	3
National appendix NA	Inside back cover

National foreword

This British Standard has been prepared under the direction of the Iron and Steel Standards Policy Committee. It is the English language version of EN 10036:1989 “*Chemical analysis of ferrous materials. Determination of total carbon in steels and irons. Gravimetric method after combustion in a stream of oxygen*”, published by the European Committee for Standardization (CEN). It supersedes BS 6200-3.8.1:1985, which is withdrawn.

Attention is drawn to the fact that this standard specifies the use of soda asbestos. In view of the hazardous nature of asbestos, a suitable alternative reagent, for example an inert ceramic impregnated with sodium hydroxide, should be used instead. A proposal to amend the text of the European Standard has been submitted to the CEN Central Secretariat.

A further method for the determination of carbon in ferrous materials has been published as BS 6200-3.8.3.

A British Standard does not purport to include all the necessary provisions of a contract. Users of British Standards are responsible for their correct application.

Compliance with a British Standard does not of itself confer immunity from legal obligations.

Summary of pages

This document comprises a front cover, an inside front cover, pages i and ii, the EN title page, pages 2 to 6, an inside back cover and a back cover.

This standard has been updated (see copyright date) and may have had amendments incorporated. This will be indicated in the amendment table on the inside front cover.

UDC 669.1:542.26:543.21

Key words: Iron- and steel products; steels; cast iron; chemical analysis; determination of content; carbon; gravimetric analysis; combustion analysis

English version

Chemical analysis of ferrous materials
Determination of total carbon in steels and irons
Gravimetric method after combustion in a stream of oxygen

Analyse chimique des matériaux
sidérurgiques — Dosage du carbone total
dans les aciers et les fontes — Méthode
gravimétrique après combustion dans un
courant d'oxygène

Chemische Analyse von Eisen- und
Stahlwerkstoffen — Ermittlung des
Gesamtkohlenstoffgehalts von Stahl und
Roheisen — Gewichtsanalytische Ermittlung
nach Verbrennung im Sauerstoffstrom

This European Standard was accepted by CEN on 15 January 1989. CEN members are bound to comply with the requirements of the CEN/CENELEC Rules which stipulate the conditions for giving this European Standard the status of a national standard without any alteration.

Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the CEN Central Secretariat or to any CEN member.

This European Standard exists in the official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to CEN Central Secretariat has the same status as the official versions.

CEN members are the national standards organizations of Austria, Belgium, Denmark, Finland, France, Germany, Greece, Iceland, Ireland, Italy, Luxemburg, Netherlands, Norway, Portugal, Spain, Sweden, Switzerland and United Kingdom.

CEN

European Committee for Standardization
Comité Européen de Normalisation
Europäisches Komitee für Normung

Central Secretariat: rue de Stassart 36, B-1050 Brussels

Brief history

This European Standard takes over the content of Euronorm 36-83 “Chemical analysis of ferrous materials — Determination of total carbon in steels and irons — Gravimetric method after combustion in a stream of oxygen”, prepared by ECISS/TC 20 “*Methods of chemical analysis*”, the Secretariat of which is allocated to the Dansk Standardiseringsrad (DS).

It has been submitted to the CEN Formal Vote following the decision of the Coordinating Commission (COCOR) of the European Committee for Iron and Steel Standardization on 1987-11-24/25.

It has been adopted and ratified by CEN BT on 1988-11-05.

According to the Common CEN/CENELEC Rules, following countries are bound to implement this European Standard:

Austria, Belgium, Denmark, Finland, France, Germany, Greece, Iceland, Ireland, Italy, Luxemburg, Netherlands, Norway, Portugal, Spain, Sweden, Switzerland and United Kingdom.

Note in clauses 1 and 9 Euronorm shall read EUROPEAN STANDARD.

Contents

	Page
Brief history	2
1 Scope and field of application	3
2 Reference	3
3 Principle	3
4 Reagents	3
5 Apparatus	3
6 Sampling	4
7 Procedure	4
7.1 Test portion	4
7.2 Blank test	4
7.3 Determination	5
8 Expression of results	5
9 Test report	5
Figure 1 — Apparatus for the gravimetric determination of the total carbon after combustion in a stream of oxygen	6
Figure 2 — Absorption bulb	6

1 Scope and field of application

This EURONORM specifies a gravimetric method for the determination of total carbon in steels and irons after combustion in a stream of oxygen.

The method is applicable to carbon contents equal to or greater than 0.1 % (m/m).

2 Reference

EURONORM 18 — Selection and preparation of samples and test pieces for steel and iron and steel products.

3 Principle

Combustion of a test portion in a stream of oxygen in a high temperature furnace (1 200-1 440 °C), with the addition of a fluxing agent to assist combustion.

Absorption of the evolved carbon dioxide in soda asbestos contained in a weighed absorption bulb.

Calculation of the carbon content from the increase in mass of the absorption bulb.

4 Reagents

During the analysis, use only reagents of recognized analytical quality.

4.1 Oxygen, cylinder oxygen, of at least 99 % purity.

4.2 Magnesium perchlorate (Anhydrone) as a drying agent.¹⁾

4.3 Fluxes: lead oxide, copper (II) oxide, tin filings: high purity iron chips of certified very low carbon content.

4.4 Copper (II) oxide, granulated.

4.5 Soda asbestos, in granules of approximately 2 mm diameter. Avoid contact with air. Handling of this reagent should take place under a fume hood with sufficient suction to avoid inhalation of asbestos dust by the operator.

4.6 Sulphuric acid, ρ 1.84 g/ml approximately. (18 mol/l approximately).

4.7 Chromic-sulphuric acid: Saturate a sulphuric acid solution, ρ 1.23 g/ml approximately (4 mol/l approximately) with chromic acid anhydride (CrO_3). The solution remains effective only as long as it retains its red colour. Sulphuric acid solution ρ 1.23 approximately, is prepared by diluting sulphuric acid ρ = 1.84 g/ml. 1 + 4 with water.

5 Apparatus

The apparatus consists of three parts: The first part includes the oxygen cylinder and the oxygen-purifier, the second part comprises the furnace and combustion tube and the third part comprises the vessels for purification and absorption of the carbon dioxide produced by combustion of the carbon in the analysis sample.

The three parts, which are interconnected by tubing and hermetically sealed stoppers, are depicted in Figure 1.

Figure 1

- A Oxygen cylinder (4.1) with a pressure regulating valve.
- B Mercury valve.
- C Furnace with non-porous porcelain tube, heated to 400 °C, containing granules of copper (II) oxide (4.4).
- D U tube containing magnesium perchlorate (4.2) and soda asbestos (4.5) separated by glass wool for drying and purification of oxygen (diameter of the tubes is 25 mm, height approximately 100 mm with connection). The U tube must be packed in such a manner that the oxygen passes first through the soda asbestos and afterwards through the magnesium perchlorate.
- E Electric resistance furnace, capable of raising the temperature of the combustion tube to 1 400 °C.
- F Thermocouple for temperature measurement. The point of the thermocouple protected by its own sheath is placed near the external surface of the combustion tube.
It is recommended that the difference between the external and the internal temperature of the tube should be checked.
- G Refractory combustion tube which is not porous at the test temperature, having an internal diameter of 20 to 30 mm and a length of at least 600 mm so that the ends of the tube remain cool during the combustion.

The tube should extend beyond each end of the furnace by not less than 150 mm.

¹⁾ Contact with organic substances should be avoided because of the potential hazard of an explosion.

- H Refractory boat with eyelet (length 80 to 100 mm, width 12 to 14 mm, height 8 to 9 mm) calcined in a current of oxygen under the working conditions.
- I,I' Small, porous refractory cylinders for protecting the end stoppers of the combustion tube against the heat. For subsequently cooling the tube, its ends can be enclosed by water-circulating lead or copper coils.
- L Glass bulb tube filled with quartz wool to trap the dust carried along by the gas flow.
- M Wash bottle containing the chromic-sulphuric acid (4.7).
- M' Drier containing the magnesium perchlorate (4.2).
- N Contact furnace with non-porous porcelain tube, heated to 400° containing copper (II) oxide granules (4.4), in order to ensure complete oxidation to carbon dioxide.
- O,O' Weighed absorption bulbs with turn off taps, for the absorption of the carbon dioxide, containing soda asbestos (4.5) and a layer (10-20 mm) of magnesium perchlorate (4.2) for retaining the water formed during the absorption of the carbon dioxide. The total mass of each absorption bulb, ready for use, should not exceed 100 g (see Figure 2).
- O'' Unweighed absorption bulb, facing the opposite way to O and O'.
- P Bottle of sulphuric acid (4.6) for the protection of the absorption bulbs against the outside atmosphere and also for monitoring the rate of the oxygen flow.

6 Sampling

Sampling shall be carried out in accordance with EURONORM 18.

The sample as prepared for analysis shall be in the form of very short chips having a thickness not exceeding a few tenths of a millimetre.

For white cast irons the analysis sample must be fine enough to pass through a sieve of 0.18 mm mesh size.

For grey cast irons the test piece shall be cut into plates 2 mm thick and broken up with pliers to avoid the possibility of errors arising from the segregation of graphite.

7 Procedure

Alter checking the leak-tightness of the apparatus and having attained a temperature of 1 200-1 400 °C in the combustion zone of the furnace (use highest temperature for the more highly alloyed steels), allow the oxygen (4.1) to flow into the apparatus for 10 to 15 minutes, at a rate of 300 to 500 ml per minute depending on the diameter of the tube used. Next disconnect the absorption bulbs and close the taps to avoid contact with ambient air. Weigh them after 10 minutes at ambient temperature and then reconnect them to the apparatus.

7.1 Test portion

Weigh the masses (m) given below as a function of presumed carbon content to the nearest 0.001 g remaining within the tolerance of ± 1.096 of the specified mass:

- a) content from 0.1 % to 1 % m approximately 2 g;
- b) content above 1 %, m approximately 1 g.

Transfer the weighed test portion to the calcined refractory boat. Add to the sample 1 to 2 g of carefully weighed flux (4.3).

7.2 Blank test

Determine the blank value of the apparatus, boat and flux by combustion of the boat containing the prescribed quantity of flux (4.3) exactly in accordance with the conditions specified for the analysis (7.3) and record the increase in mass (mass m_0) of the absorption bulb.

Where there is any doubt about the purity of the boat, this should be verified by the combustion in the boat of the exact amount of flux used in the analysis, together with 1 g of high purity iron of certified very low carbon content (4.3). In this case, the blank value (mass m_0) is obtained after correcting for the certified carbon content of the high purity iron.

The leak-tightness of the apparatus and the effectiveness of the purification system can be checked without submitting materials and fluxes to combustion.

7.3 Determination

Cut off the oxygen flow, then open the combustion tube at the end where the oxygen enters and introduce the boat with the sample into the middle of the heated zone of the tube by means of a rigid nickel rod. Close the tube immediately and after one minute allow an oxygen flow to pass through at a rate of 300 to 500 ml per minute depending on the diameter of the tube used.

Combustion should be complete after approximately 2 minutes but continue the oxygen flow for a further 15 to 20 minutes to ensure the complete expulsion of the carbon dioxide from the combustion tube and the purification bulbs.

Cut off the oxygen flow, close the taps of the weighed absorption bulbs and remove the refractory boat from the combustion tube. Check whether the combustion has been properly carried out by examining the fused mass in the boat withdrawn from the furnace. Complete combustion is indicated by a totally fused mass in which no traces of the original sample can be recognized.

Disconnect the absorption bulbs and after 10 minutes weigh them at ambient temperature.

The increase in mass represents the carbon dioxide absorbed (mass m_1).

8 Expression of results

The percentage by mass of carbon (C) is given by the expression:

$$\text{C \%} = \frac{(m_1 - m_0) \times 27.29}{m}$$

where

- m_1 is the mass of carbon dioxide from the test sample, in g;
- m_0 is the mass of carbon dioxide from the blank test, in g;
- m is the mass of the test portion, in g;
- 27.29 is the conversion factor of carbon dioxide to carbon. multiplied by 100.

9 Test report

The test report shall contain the following particulars:

- a) the method of analysis used by reference to this Euronorm;
- b) the results obtained, as well as the form in which they are expressed;
- c) any particular details which may have been noted during the determination;
- d) any operations not specified in this Euronorm or any optional operations which could have had an influence on the result.

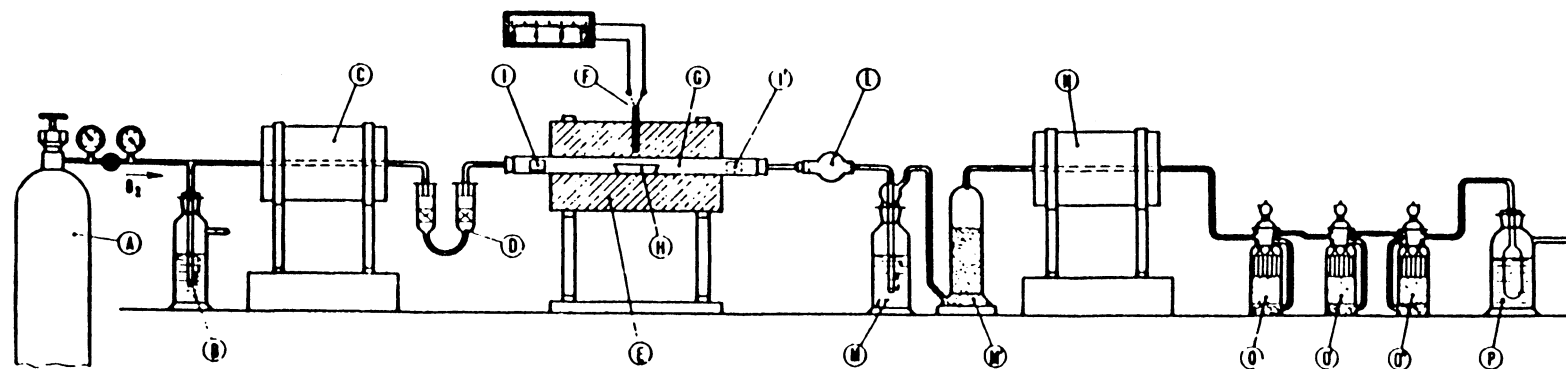


Figure 1 — Apparatus for the gravimetric determination of the total carbon after combustion in a stream of oxygen

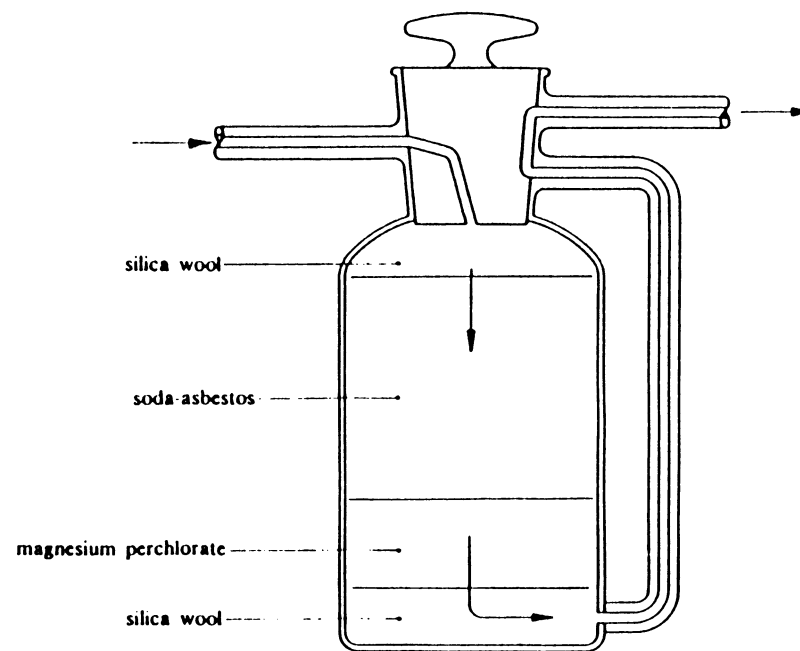


Figure 2 — Absorption bulb

National appendix NA

The United Kingdom participation in the preparation of this European Standard was entrusted by the Iron and Steel Standards Policy Committee (ISM/-) to Technical Committee ISM/18 upon which the following bodies were represented:

BCIRA

British Forging Industry Association

British Steel Industry

Department of Trade and Industry (Laboratory of the Government Chemist)

Ferro Alloys and Metals Producers' Association

Ministry of Defence

BSI — British Standards Institution

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

Revisions

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover.
Tel: 020 8996 9000. Fax: 020 8996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

Buying standards

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services. Tel: 020 8996 9001. Fax: 020 8996 7001.

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

Information on standards

BSI provides a wide range of information on national, European and international standards through its Library and its Technical Help to Exporters Service. Various BSI electronic information services are also available which give details on all its products and services. Contact the Information Centre.
Tel: 020 8996 7111. Fax: 020 8996 7048.

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration.
Tel: 020 8996 7002. Fax: 020 8996 7001.

Copyright

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

If permission is granted, the terms may include royalty payments or a licensing agreement. Details and advice can be obtained from the Copyright Manager.
Tel: 020 8996 7070.